


## Arms Case Example #9

These images are examples of the Renuvion<sup>®</sup> device used as a tool for coagulation<sup>1</sup> resulting in tissue contraction<sup>2,3,4,5,6</sup>. As with any procedure, individual results may vary.

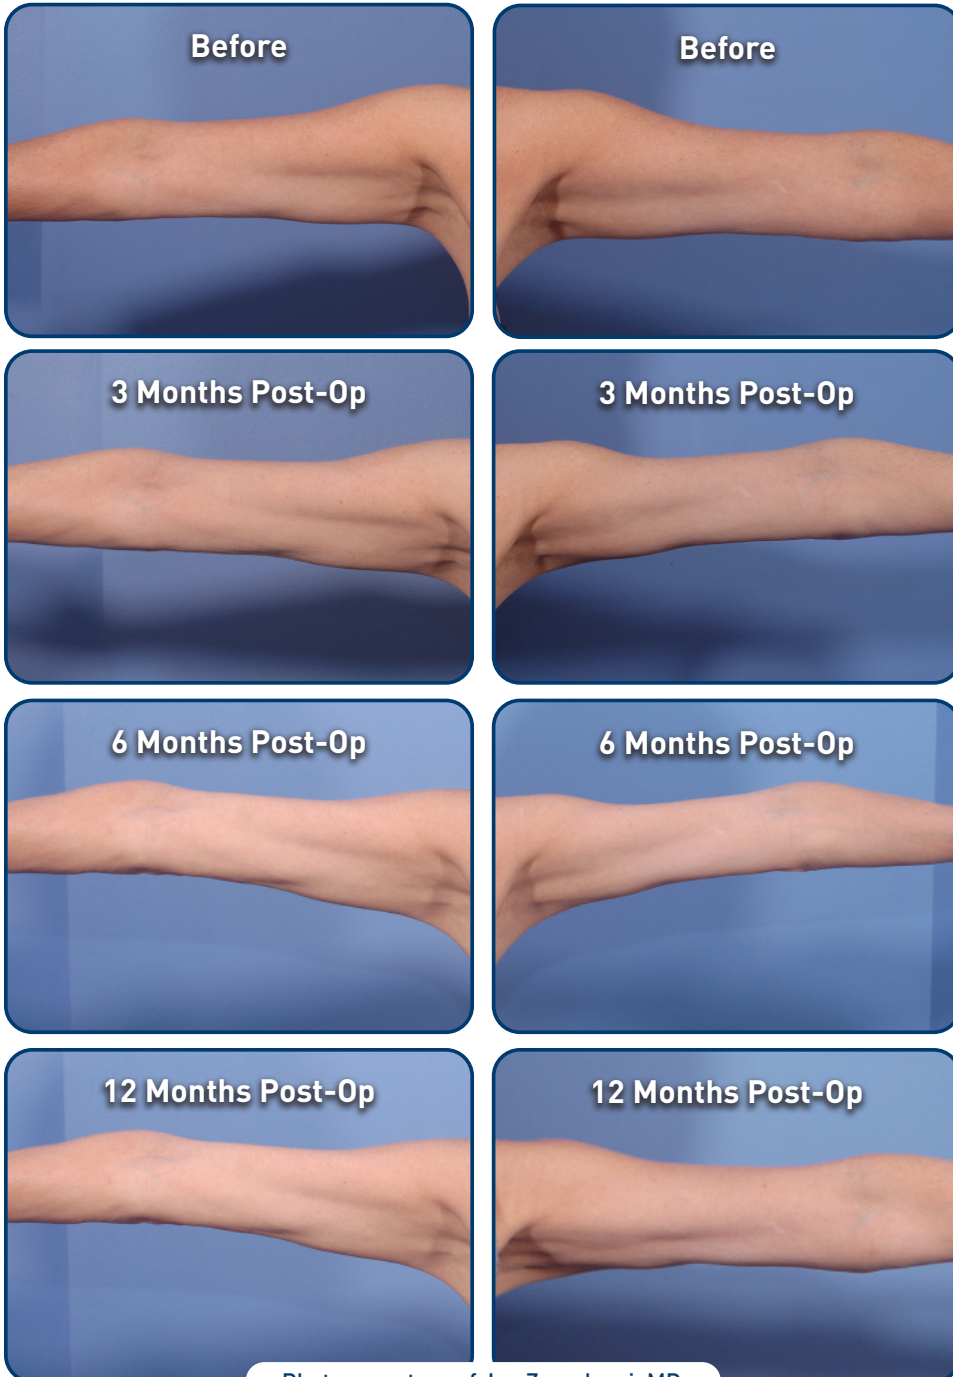

Photos courtesy of Jan Zemlenyi, MD

**Patient:**

60-year-old female

**Procedure Type:**

Traditional liposuction

**Amount of  
Fat Removed:**

50cc

**Renuvion used  
subdermally on arms**



Photos courtesy of Jan Zemplyni, MD

**Patient:**  
60-year-old female

**Procedure Type:**  
Traditional liposuction

**Amount of Fat Removed:**  
50cc

**Renuvion used subdermally on arms**

The Renuvion system is intended to be used for the coagulation of soft tissue during open surgical procedures, and has received a general clearance and has not been determined to be safe or effective for use in any specific indication or anatomical location.

As with all energy devices there are inherent risks associated with its use. For additional information related to the intended use, risks and references cited please visit [Renuvion.com/DisclosuresB](https://renuvion.com/disclosuresB).